

**Test Report**

Number: SZHH01672938

Applicant: GIGACLOUD TECHNOLOGY (USA) INC.  
18961 ARENTH AVENUE CITY OF INDUSTRY  
CA 91748

Date: Jun 28, 2022

Attn: Mr. Joseph

**Sample Description:**

One (1) set of submitted sample said to be :

Item Name : **Bunk Bed.**  
Item No. : **WF291471, WF291472.**  
Labelled Age Group : Not Specified.  
Applicant's Specified Age : Over 6 years.  
Grading for Testing :  
Packaging Provided by : No.  
Applicant :  
Additional Material and Wet : Yes.  
Paint Provided :  
Country of Origin : China.  
Country of Destination : United States.  
Date Sample Received : Apr 08, 2022 & May 08, 2022 & Jun 08, 2022 & Jun 28, 2022 .  
Testing Period : Apr 08, 2022 – Jun 28, 2022.

**SZHH01672938**



**Tests conducted:**

As requested by the applicant, refer to attached page(s) for details.



Page 1 of 14

**Test Report**

Number: SZHH01672938

Conclusion:

Tested Samples  
Submitted samples

Standard

ASTM F1427-21<sup>§1</sup> - Standard Consumer Safety Specification for Bunk Beds

Result  
Pass

16 CFR Part 1513 - Requirements for Bunk Beds Intended for Use by Children /  
16 CFR Part 1213 -Requirements for Bunk Beds not Intended for Use by Children

Pass

Consumer Product Safety Improvement Act (CPSIA) 2008 Section 103  
Tracking labels for children products

See test conducted

U.S. CFR Title 16 (CPSC Regulations)  
Mechanical and physical test

Pass

Requirement

U.S. CFR Title 16 (CPSC Regulations) Part 1500.3(c)(6)(vi)  
flammability test on rigid and pliable solids

Result  
Pass

Tested components of  
submitted samples

Standard

U.S. CFR Title 16 Part 1303 total Lead content

Result  
Pass

U.S. Consumer Product Safety Improvement Act 2008 Title I, Section 101 for total Lead content in surface coating

Pass

U.S. Consumer Product Safety Improvement Act 2008 Title I, Section 101 for Total Lead content in Non-surface coating materials (substrate)

Pass

Test Item

Applicant's requirement with reference to US Consumer Product Safety Improvement Act 2008 Title I, Sec 108(a) & (b)(3) and US 16 CFR Part 1307 for Prohibition of Children's Toys and Child Care Articles Containing Specified Phthalates

Result  
Pass

Authorized by:  
For Intertek Testing Services Shenzhen Ltd  
Xiamen Branch



Rachel L. Guo  
General Manager



Page 2 of 14

Intertek Testing Services Shenzhen Ltd. Xiamen Branch  
深圳天祥质量技术服务有限公司厦门分公司

Unit 1E,1st floor,Unit 2C,2nd floor,Unit 4C  
、4D、4L、4O, 4th floor, Xinglian  
Building, No.2, Chuangxin RD, Huoju Hi-  
tech District, Xiamen, Fujian, P.R.C  
福建省厦门市湖里区火炬高新区创新路 2  
号兴联电子大厦一楼 1E 区,二楼 2C 和四楼  
4C、4D、4L、4O

Tel:+86592 8063339  
Fax:+86592 8060054  
[www.intertek.com](http://www.intertek.com)  
[www.intertek.com.cn](http://www.intertek.com.cn)



**Test Report**

Number: SZHH01672938

Tests Conducted

1. Safety Specification for Bunk Beds

Reference standard: ASTM F1427-21<sup>§1</sup> - Standard Consumer Safety Specification for Bunk Beds.

Note: Lead in paints per 16 CFR 1303 is stated in this standard but not covered in the following test result.

Number of sample tested: One (1) piece.

Executive summary:

Clause	Testing Items / Requirements	Assessment
1	Scope	
2	Referenced documents	
3	Terminology	
4	Performance requirements	
4.1	Vertical protrusions	
4.1.1	All vertical protrusions along the top inside surfaces of any individual component (including but not limited to bed end structures and guard rails) of the upper bunk shall not extend more than 3/16 in. (4.8 mm) above the upper edge of the adjacent surface. Ladder stiles (uprights) shall not extend more than 3/16 in. (4.8 mm) above the upper edge of the adjacent surface.	P
4.1.2	Any cap used along the top surface of the upper bunk shall not have a vertical protrusion greater than 3/16 in. (4.8 mm) at the edge of the protrusion above the upper edge of the adjacent surface. If the cap is flush with or overhangs the edge of the corner post or other vertical protrusion, the maximum vertical protrusion shall not exceed 3/16 in. (4.8 mm). The cap shall have a maximum height of no more than 20 % of the width or diameter of the cap. At no point shall the cap overhang the post more than 1/16 in. (2 mm). The cap shall fit flush with the top of the corner post.	P
4.2	Fit of top bed to bottom bed  The bed post shall be designed so that the minimum height of lift to allow horizontal disengagement of the top bed from the bottom bed shall be 1-1/4 in. (32 mm), or a fastening mechanism may be used that will prevent the disengagement of the top bed from the bottom bed.	NA



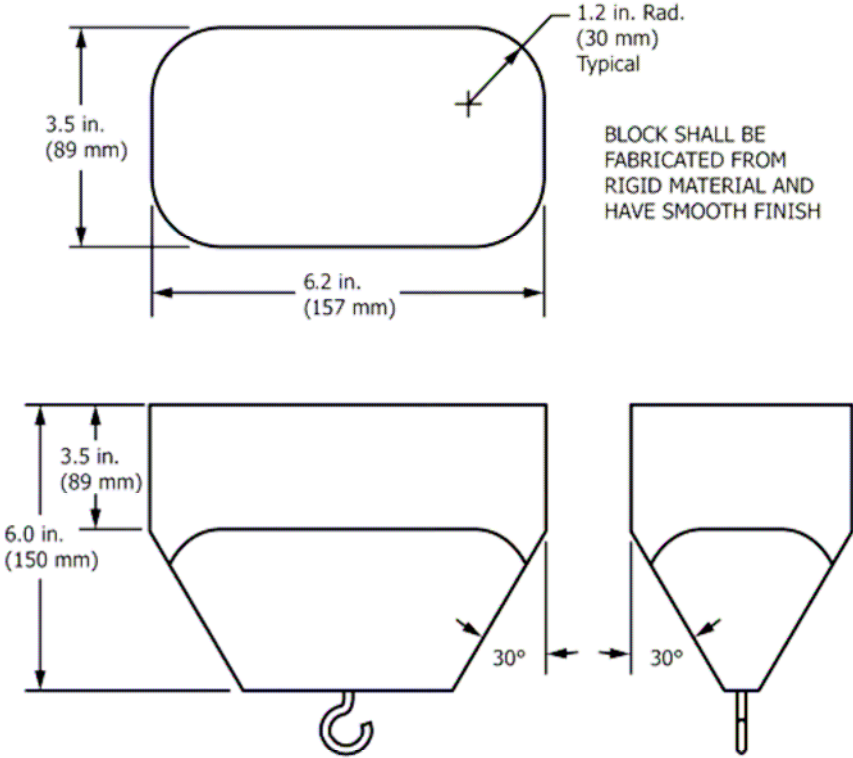
Page 3 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

Clause	Testing Items / Requirements	Assessment
4.3	<p>Mattress and foundation size and fit (top bed)</p> <p>There shall be no gaps between the interior bed structure and the edges of the mattress and foundation that will permit complete passage of the wedge block shown in Fig. 5 when tested in accordance with 5.2.</p>  <p><b>FIG. 5 Wedge Block for Tests in Section 5</b></p>	P
4.4	<p>Mattress size and fit (lower foundation)</p> <p>There shall be no space, between the edge of the manufacturer's recommended mattress and the interior boundary of any component(s) attached to lower bunk (for example, ladders, book shelves, desk), greater than 1.88 in. (48 mm) and smaller than 9 in. (229 mm), when tested in accordance with 5.3.</p>	P
4.5	Upper and lower foundation support systems	
4.5.1	<p>The foundation support system shall confine the horizontal position of the mattress and the foundation and shall prohibit the mattress and foundation from falling when the mattress or foundation is manipulated.</p>	P

**Test Report**

Number: SZHH01672938

Tests Conducted

Clause	Testing Items / Requirements	Assessment
4.5.2	In the event cross-members are utilized, a minimum of two per bed are required. If more than two cross-members are utilized, they shall be spaced so that the distance between adjacent cross-members or between the cross-members and the bed end structures will not permit complete passage of the wedge block or will allow complete passage of both the wedge block and a 9-in. (229 mm) diameter rigid sphere when tested in accordance with 5.9.	P
4.5.3	The foundation support system shall not be capable of being dislodged without the release of positive fastening devices or the use of hand tools.	P
4.5.4	The foundation support system shall not fail when tested in accordance with 5.4.	P
4.6	Side Rails	
4.6.1	Bolt-On Side Rail, that attach at their ends or on their side to the bed post, shall be secured at each end by two bolts with a minimum size of 1/4 in. (6.4 mm) diameter or ISO/ANSI size M6. For wood beds, these bolts shall be spaced a minimum of 1-1/2 in. (38 mm) apart on their centers. When the bolts are fully tightened in the assembled bed, no more than 1/4 in. (6.4 mm) of thread shall be exposed.	P
4.6.2	Hook-On Side Rails, securely attached to the bed post. Hook-on attachments shall require an additional action other than an upwards force to disengage.	NA
4.6.3	Side rail attachments  There shall be no structural failure of bed side rail fastening systems when tested in accordance with 5.5.	P
4.7	Guardrails	
4.7.1	Two guardrails shall accompany any bed in which the underside of the foundation is over 30 in. (762 mm) from the floor. Guardrails may be separate from or integral with the ladder.	P
4.7.2	Guardrails shall be attached in a manner that requires the intentional release of a fastening device or be so designed that they cannot be removed unless forces are applied sequentially in different directions.	P
4.7.3	The upper edge of the guardrails shall be at least 5 in. (127 mm) above the sleeping surface when a mattress of a thickness that is the maximum specified by the manufacturer's instructions is used on the bed.	P
4.7.4	With no mattress on the bed, there shall be no openings in the rigid bed structure below the lower edge of any opening of the guardrail that would permit complete passage of the wedge block shown in Fig. 5 when tested in accordance with 5.6.	P



Page 5 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

Clause	Testing Items / Requirements	Assessment
4.7.5	A guardrail may terminate before reaching the bed end structure, providing there is no more than 15 in. (381 mm) between either end of the guardrail and the bed end structures in the same plane when measured at a point 5 in. (127 mm) above the sleeping surface as established by the maximum mattress thickness specified by the manufacturer. The second guardrail may terminate before reaching the bed end structure. If this guardrail terminates before reaching the bed end structure, there shall be no more than 0.22 in. (5.6 mm) between either end of the guardrail and the bed end structure when measured horizontally between the bed end structure and the nearest point on the guardrail.	P
4.8	Bed structure	
4.8.1	The upper edge of the upper bunk end structures for at least 50 % of the distance between the two posts at the head and foot of the upper bunk shall be at least 5 in. (127 mm) above the sleeping surface when a mattress and foundation of the maximum size and thickness specified by the manufacturer's instructional literature is used on the upper bunk.	P
4.8.2	There shall be no openings in the rigid end structures of the upper bunk/bunks that will permit the free passage of the wedge block shown in Fig. 5 when tested in accordance with 5.7.1. This requirement shall apply only to that portion of the bed end structure that is above the foundation support system of the upper bunk/bunks.	P
4.8.3	When tested in accordance with 5.7.2, there shall be no openings within the entire boundary of the lower bunk that will permit free passage of the wedge block shown in Fig. 5, unless they are large enough to permit the free passage of a 9 in. (229 mm) diameter rigid sphere. This requirement does not apply to openings that are below the level of the lower bunk foundation support system. This requirement shall apply to that portion of the bed structure that is between the level of the lower bunk foundation support system and the level of the upper bunk foundation support system. Such openings include, but are not limited to, bed end structures, foundation, ladders, desks, or bookshelf components, or a combination thereof, as offered with the bed for purchase and designed to be attached to the bed structure.	P
4.8.4	When tested in accordance with 5.7.2.3 and 5.7.2.4, all portions of the boundary of any opening of the entire lower bunk boundary that permits free passage of a 9 in. (229 mm) diameter rigid sphere also must conform to the neck entrapment requirement.	P
4.9	Ladders	
4.9.1	A lean-on (slanted) or hang-on (vertical) ladder shall be supplied with each bunk bed set or the ladder may be incorporated as part of the bed structure. The ladder may be separate from or integral with the guardrail. The ladder shall be attached in a manner that prevents inadvertent disengagement, repositioning, or tilting while in use.	P



Page 6 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

Clause	Testing Items / Requirements	Assessment
4.9.2	There shall be no openings between ladder structures that allow complete passage of the wedge block shown in Fig. 5, unless they are large enough to permit the free passage of the 9 in. (229 mm) diameter rigid sphere. The width of the ladder shall be no less than 10 in. (254 mm) measured from the inside of the stiles. Vertical spacing of ladder steps shall be no greater than 12 in. (305 mm) when measured from the floor to the first step or between steps. When bed structures are used as ladders, vertical spacing may be up to 16 in. (407 mm).	P





## Test Report

Number: SZHH01672938

### Tests Conducted

Clause	Testing Items / Requirements	Assessment
4.9.3	There shall be no openings between the ladder step and the upper bunk boundary that allow complete passage of the wedge block shown in Fig. 5, unless they are large enough to permit the free passage of the 9 in. (229 mm) diameter rigid sphere.	P
4.9.4	For ladders attached to the side of the lower bed and for which mattress height is above the side rail, there shall be no gaps between the edge of the manufacturers recommended mattress and the interior vertical stile between 1.88 in. (48 mm) and 9 in. (229 mm) when tested in accordance with 5.3.	P
4.10	Metal beds: frame and fastenings  There shall be no separation of any of the attachments of the foundation support system to the end structures of the bed when tested in accordance with 5.8.1.1 and 5.8.2.	P
5	Test methods	
6	Marking and labeling	P
7	Instructional literature	P

Abbreviation: P = Pass; NA = Not Applicable

## 2. 16 CFR Part 1513-Requirements for Bunk Beds Intended for Use by Children/16 CFR Part 1213-Requirements for Bunk Beds Not Intended for Use by Children

With reference to 16 CFR Part 1513 - Requirements for Bunk Beds & 16 CFR Part 1213 - Safety Standard for Entrapment Hazards in Bunk Beds.

### Executive summary:

Clause	Requirements	Assessment
1513.3(a)/1213.3(a)	Guardrails	
(1)	Any bunk bed shall provide at least two guardrails, at least one on each side of the bed, for each bed having the underside of its foundation more than 30 inches (760 mm) from the floor.	P
(2)	One guardrail shall be continuous between each of the bed's end structures. "Continuous" means that any gap between the guardrail and end structure shall not exceed 0.22 inches (5.6 mm) (so as to not cause a finger entrapment hazard for a child).	P
(3)	The other guardrail may terminate before reaching the bed's end structures, providing there is no more than 15 inches (380 mm) between either end of the guardrail and the nearest bed end structures.	P
(4)	For bunk beds designed to have a ladder attached to one side of the bed, the continuous guardrail shall be on the other side of the bed.	P
(5)	Guardrails shall be attached so that they cannot be removed without either intentionally releasing a fastening device or applying forces sequentially in different directions.	P
(6)	The upper edge of the guardrails shall be no less than 5 inches (130 mm) above the top surface of the mattress when a mattress of the maximum thickness specified by the bed manufacturer's instructions is	P



Page 8 of 14





**Test Report**

Number: SZHH01672938

Tests Conducted

Clause	Requirements	Assessment
	on the bed. This requirement does not prohibit a wall-side guardrail that terminates in a quarter-circle bend and attaches to the side rail of the upper bunk foundation.	
(7)	With no mattress on the bed, there shall be no openings in the structure between the lower edge of the uppermost member of the guardrail and the underside of the upper bunk's foundation that would permit passage of the wedge block shown in Figure 1 of this part when tested in accordance with the procedure at §1513.4(a)/1213.4(a).	P
1513.3(b)/1213.3(b)	Bed end structures	
(1)	The upper edge of the upper bunk end structures shall be at least 5 inches (130 mm) above the top surface of the mattress for at least 50 percent of the distance between the two posts at the head and foot of the upper bunk when a mattress and foundation of the maximum thickness specified by the manufacturer's instructions is on the bed.	P
(2)	With no mattress on the bed, there shall be no openings in the end structures above the foundation of the upper bunk that will permit the free passage of the wedge block shown in Figure 1 when tested in accordance with the procedure at §1513.4(b)/1213.4(b).	P
(3)	When tested in accordance with §1513.4(c)/1213.4(c), there shall be no openings in the end structures between the underside of the foundation of the upper bunk and upper side of the foundation of the lower bunk that will permit the free passage of the wedge block shown in Figure 1, unless the openings are also large enough to permit the free passage of a 9-inch (230-mm) diameter rigid sphere.	P
(4)	All portions of the boundary of any opening required by §1513.4(c)(1) and (2)/1213.4(c)(1) and (2) to be probed by the wedge block of Figure 1, and that permits free passage of a 9-inch diameter sphere, must conform to the neck entrapment requirements of §1513.4(c)(3)/1213.4(c)(3).	P
1513.5/1213.5	Marking and labeling	P
1513.6/1213.6	Instructions	P

Abbreviation: P = Pass; NA = Not Applicable



Page 9 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

3 Tracking Label Assessment

As per Consumer Product Safety Improvement Act (CPSIA) 2008 Section 103 Tracking labels for children products

Tracking label found on the product:



Name of importer	GIGACLOUD TECHNOLOGY(USA) INC.
Location of production	XYX
Date code	April Month 2022 Year

Remark: As requested by the applicant, the tracking label information on the packaging was not assessed.

Note: The tracking label assessment was based on the submitted sample and the information provided by the applicant. There was no verification on the validity of such information.

**Test Report**

Number: SZHH01672938

Tests Conducted

4 Physical and Mechanical Test

As per U.S. Code of Federal Regulations Title 16 Part 1500.50, the hazards of sharp points, sharp edge and small parts are assessed both before and after applicable use and abuse tests.

Conclusion:	No. of Sample Tested	Sharp Point (1500.48)	Sharp Edge (1500.49)	Small Part (1501)
As received	1	P	P	NA
Impact (1500.53(b))	1	P	P	NA
Flexure (1500.53(d))	0	NA	NA	NA
Torque (1500.53(e))	1	P	P	NA
Tension (1500.53(f))	1	P	P	NA
Compression (1500.53(g))	1	P	P	NA

Remark :P = Pass NA= Not Applicable

5 Flammability Test

Test requirement: U.S. Code of Federal Regulations Title 16 Part 1500.44 for rigid and pliable solids.

Result: Did not ignite



Page 11 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

6 Total Lead (Pb) Content in Surface Coating (U.S. 16 CFR Part 1303 and CPSIA Section 101)

As per Standard Operating Procedure for Determining Lead (Pb) in paint and other similar surface coatings, test method CPSC-CH-E1003-09.1 was used and total Lead content was determined by Inductively Coupled Argon Plasma Spectrometry.

Element	Result (ppm)			Reporting Limit (ppm)	Limit (ppm)
	Tested Component				
	(1)	(6)	(8)		
Lead (Pb)	46	ND	ND	10	90

The above limit was quoted according to U.S. CFR Title 16 Part 1303 and U.S. Consumer Product Safety Improvement Act 2008 Title I, Section 101 for total Lead content in surface coating.

ppm = parts per million = mg/kg

ND = Not detected (less than reporting limit)

Tested components: See component list in the last section of this report

7 Total Lead (Pb) Content in Non-Surface Coating Materials (Substrate) (U.S. CPSIA Section 101)

As per Standard Operating Procedures for Determining total Lead (Pb) in children's products, test methods CPSC-CH-E1002-08.3 and/or CPSC-CH-E1001-08.3 were used and total Lead content was determined by Inductively Coupled Argon Plasma Spectrometry.

Element	Result (ppm)				Reporting Limit (ppm)	Limit (ppm)
	Tested Component					
	(2)	(3+4)	(5)	(9)		
Lead (Pb)	13	ND	ND	ND	10	100

The above limit was quoted according to U.S. Consumer Product Safety Improvement Act 2008 Title I, Section 101 for total Lead content in Non-surface coating materials.

ppm = parts per million = mg/kg

ND = Not detected (less than reporting limit)

Tested components: See component list in the last section of this report



Page 12 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

8 Phthalate Content (U.S. 16 CFR Part 1307)

As per CPSC-CH-C1001-09.4, by Gas Chromatographic-Mass Spectrometric (GC-MS) analysis.

Test item	CAS No.	Result (%) $\theta$	Reporting limit (%)	Limit (%)
		Tested component		
		(1) (2) (6) (7) (8) (9)		
Dibutyl phthalate (DBP)	84-74-2	ND	0.01	0.1
Di-(2-ethyl hexyl) phthalate (DEHP)	117-81-7	ND	0.01	0.1
Benzyl butyl phthalate (BBP)	85-68-7	ND	0.01	0.1
Di-iso-nonyl phthalate (DINP)	28553-12-0/ 68515-48-0	ND	0.01	0.1
Diisobutyl phthalate (DIBP)	84-69-5	ND	0.01	0.1
Di-n-pentyl Phthalate (DPENP)	131-18-0	ND	0.01	0.1
Di-n-hexyl Phthalate (DHEXP)	84-75-3	ND	0.01	0.1
Dicyclohexyl Phthalate (DCHP)	84-61-7	ND	0.01	0.1

The above limit was quoted according to U.S. 16 CFR Part 1307 for Prohibition of Children's Toys and Child Care Articles Containing Specified Phthalates.

ND = Not detected (less than reporting limit)  
 $\theta$  = Single result for each test component/group

Tested Components: See component list in the last section of this report

Component list:

- (1) Black coating on metal (surface of frame)
- (2) Black plastic (bottom cap of frame)
- (3) Silver color metal excluding black coating (round tube & rect tube & sheet frame)
- (4) Black treated metal (all screws for frame)
- (5) Silver color solder excluding black coating (joint)
- (6) Black coating on paper (warning label on frame)
- (7) White paper with adhesive (warning label on frame)
- (8) Black coating on plastic (cover of board)
- (9) White plastic excluding coatings (cover of board)

\*\*\*\*\*

End of report



Page 13 of 14



**Test Report**

Number: SZHH01672938

Tests Conducted

*The statements of conformity reported have considered the decision rule agreed, namely that Intertek have taken account of measurement uncertainty as calculated by Intertek, and applied according to ILAC-G8/09:2019 (Non-binary acceptance based on guard band  $w = U$ ) except designation from the customer, regulation or test specification. This decision rule only applies to the numeric test results.*

*The sample(s) and sample information hereto are provided by the client who shall be solely responsible for the authenticity and integrity thereof. The results shown in this report relate only to the sample(s) received and tested. It is not intended to be a recommendation for any particular course of action. Intertek does not accept a duty of care or any other responsibility to any person other than the Client in respect of this report and only accepts liability to the Client insofar as is expressly contained in the terms and conditions governing Intertek's provision of services to you. Intertek makes no warranties or representations either express or implied with respect to this report save as provided for in those terms and conditions. We have aimed to conduct the review on a diligent and careful basis and we do not accept any liability to you for any loss arising out of or in connection with this report, in contract, tort, by statute or otherwise, except in the event of our gross negligence or wilful misconduct. This report shall not be reproduced unless with prior written approval from Intertek.*



Page 14 of 14

**Intertek Testing Services Shenzhen Ltd. Xiamen Branch**  
深圳天祥质量技术服务有限公司厦门分公司

Unit 1E, 1st floor, Unit 2C, 2nd floor, Unit 4C  
、4D、4L、4O, 4th floor, Xinglian  
Building, No.2, Chuangxin RD, Huoju Hi-  
tech District, Xiamen, Fujian, P.R.C  
福建省厦门市湖里区火炬高新区创新路2  
号兴联电子大厦一楼1E区, 二楼2C和四楼  
4C、4D、4L、4O

Tel: +86592 8063339  
Fax: +86592 8060054  
**www.intertek.com**  
**www.intertek.com.cn**

