



Assembly Instructions

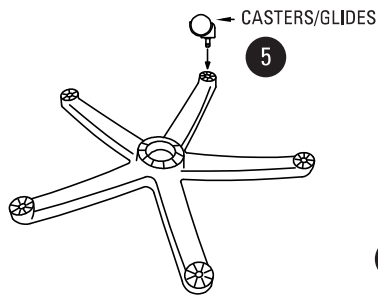


FIGURE 1.

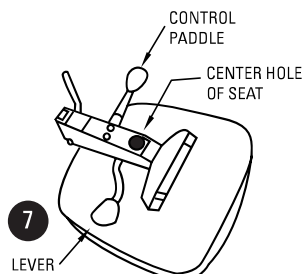


FIGURE 2.


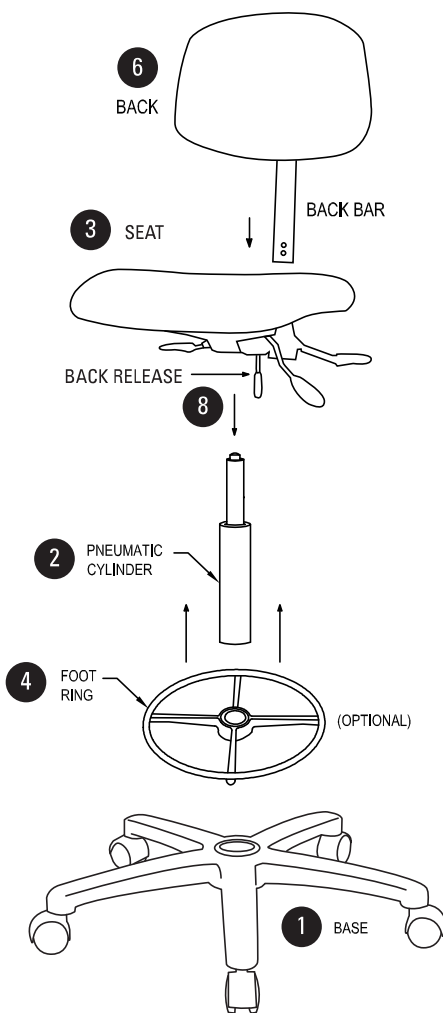


FIGURE 3.

- 1) Remove base, back/back bar, pneumatic cylinder, seat, foot ring (if included) and casters/glides from box.
- 2) Place base (1) upside down and insert casters/glides (5) (see figure 1).
- 3) Slide **optional** foot ring (4) over bottom pneumatic cylinder (2). The foot ring rests atop spokes. Make sure spokes face the floor.
- 4) Flip the base so casters/glides are on the floor and insert pneumatic cylinder (2) as shown in (figure 3) into center hole of base with colored button up. Lightly push down. Adjust foot ring to desired height.
- 5) Align the center hole of the underside of the seat assembly (3) with the top of the pneumatic cylinder (2) and lightly push down. Kneel on the seat to hold it together. This will press the base, pneumatic cylinder and seat together. (Underside of the seat is shown in Figure 2)
- 6) Lift the back release. Insert back bar through the control channel slot. Adjust the height of the seat back for comfort and push the back release lever down to lock the bar in place. Once locked, push the enclosed safety button into the lower hole of back bar, flat side out.
- 8) Adjust the seat back to the desired angle using the control lever located on the side of the seat. You can adjust the height of the back by lifting the back release up. Push the back release(8) down to lock the bar in place.
- 9) To raise the height of your chair, take your weight off of the chair and pull up on the lever (7) on the underside of the seat and adjust.
- 10) To lower the height of your chair you must be seated with your weight on the seat, lift up on lever (7).



Assembly Instructions

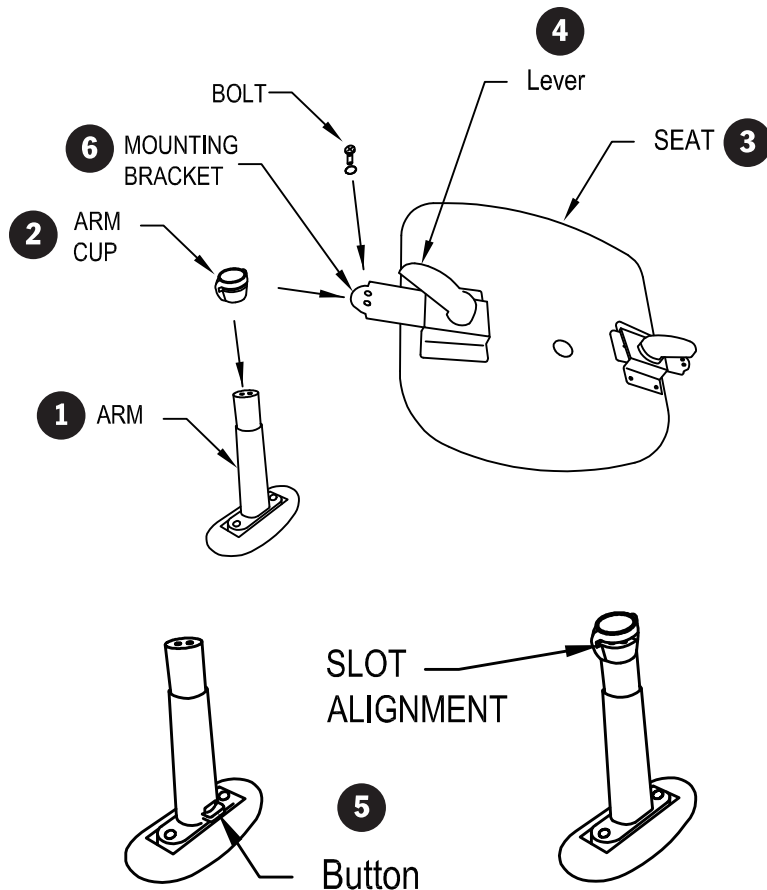

- 1) Remove the two bolts from the (1) arm.
- 2) Align the open slot of the (2) arm cup so that it is even with the bottom of the cylinder of (1) arm.
- 3) With the (3) seat upside down, align the slot of the (2) arm cup with the (6) mounting bracket. Attach with the two bolts. (Note: Make sure that the (5) button is facing away from the (3) seat.) Repeat steps for opposite side.
- 4) You can adjust the arms in and out by loosening (4) lever and sliding the arm in or out. When adjusted to desired location, tighten (4) lever.
- 5) You can adjust the arms up or down by pulling up on (5) button, adjust to desired height and then release (5) button.

Lab Grade Seating Cleaning Protocol

1. Dry-clean surfaces with a clean cloth to remove loose dirt/dust/organic material
2. Wet-clean surfaces with warm water and a mild detergent, scrubbing where necessary to remove stubborn dirt and contamination
3. Rinse surfaces with clean water and cloth – **do not use high pressure spray equipment** as this may force liquids into gaps and crevices where chair parts meet
4. Manually dry, or allow the area to dry completely
5. Apply disinfectant/cleaning solution at the recommended concentration for the appropriate contact time. **Do not apply solution at a rate higher than the recommended concentration and do not allow to contact for longer than the recommended contact time. Doing so may result in degradation of upholstery, plastic and rubber parts, or create conditions that will lead to corrosion of metal parts. These outcomes will result in early failure of chair parts and may negate the manufacturer's warranty.**
6. Wet-clean surfaces with warm water and a mild detergent which is extremely important for surfaces that are susceptible to damage from the disinfectant/cleaner chemicals
7. Rinse the chair again with clean water/cloth
8. Manually dry, or allow the area to dry completely
9. In high risk areas, repeat steps 5 through 8 above with a wide spectrum disinfectant

NOTES:

- For proper cleaning, start the cleaning protocol from the top of the chair/stool and proceed to the bottom to assure any cleaning solutions and dirt/contamination are removed should they drip or fall to lower parts of the chair
- **Do not clean oil/grease from the shaft of height-adjustable gas springs or pneumatic pistons as this will interfere with their ability to work over time, and result in shortened lifetime or failure**

This recommended cleaning protocol should in no way conflict with any other stated cleaning process as defined by governmental or corporate regulations. It is, however, a recommended process to assure long-term wear of laboratory chairs and stools in these challenging environments.