ADJUSTABLE BED BASE
USER MANUAL



Please read the manual carefully and keep it safe for future maintenance.

Contents

Safety & Warranty Warnings	01
Overview & Parts List	03
Installation Guide	05
Remote Control Instructions	07
Pairing Remote Control Instructions	08
Synchronizing Two Bases - Unison Movement	09
Tandem Bracket Installation	10
Troubleshooting	11

Safety & Warranty Warnings

ATTENTION:
Read the following information before using this product. Failure to use a surge protection device could compromise safety or cause product malfunction and could void the electrical portion of your warranty.

Electrical surges are by far the biggest cause of problems with electrical circuits. In order to help protect your investment in case of a power surge or outage, use a surge protection device (not included).

WARRANTY WARNING!
Do not open or tamper with the transformer, control box, motors, or remote control (with the exception of battery compartments). The product warranty will be void if these components are tampered with.

SMALL CHILDREN AND PETS:
Immediately dispose of all packing materials as they can smother small children and pets. Do not allow any persons or pets under the bed. Children, convalescents and disabled person should not operate the bed without adult supervision.

HOSPITAL OR CONVALESCENT USE DISCLAIMER:
Adjustable beds are designed and engineered for a life style of in-home comfort and are not intended for hospital use or for a bed-ridden patient on an extended recovery. Adjustable beds are not equipped with bars to help patients get safely in and out of bed and are not intended to be used around tent type oxygen therapy or explosive gases.

PACEMAKER WARNING:
Electronics may activate a special sensor in your pacemaker that detects motion. This can fool the pacemaker into “thinking” you are engaged in some sort of physical activity and require a faster heart rate. You may experience a sensation similar to when you are exercising. Consult your physician for further information.

Safety & Warranty Warnings

WEIGHT UNITS
The limitation for this adjustable bed is 750 lbs. The bed will structurally support these weights, provided the weight is evenly distributed across the head and foot sections. This product is not designed to support or lift this amount in the head or foot section alone. Exceeding this weight restriction could damage the bed and/or cause injury and void the warranty. Enter or exit the bed in a flat position and do not sit on the head or foot sections while in the raised position.

LIFTING AND LOWERING MECHANISMS AND MASSAGE UNITS:
It is normal for the raising and lowering feature on this bed to emit a minimal humming sound during operation.

LOCATION ENVIRONMENT:
The level of sound experienced in a room is directly related to the environment within that location. In a room with hardwood floors and the massage units turned on, a vibrating noise can be noticeable. To reduce the resonance, place a piece of carpet or rubber casters cups under the legs. The rubber caster cups also prevent the bed from sliding when located on smooth or hard surface flooring.

TO REDUCE THE RISK OF SHOCK, BURNS, FIRE OR INJURY:
Make sure the base is in a flat position and the vibrating motors are turned off before unplugging the bed base from the power source. Always unplug the base from the electrical outlet before cleaning or servicing the base. If the cord or plug is damaged, discontinue use of the bed base.

FCC COMPLIANCE:
This device complies with part 15 of the FCC Rules for residential use. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Radio Frequency: 2.4 GHz

Overview & Parts List

All electronics and components that need to be installed are located in boxes.
Before discarding the packing materials, ensure that all the parts are accounted for.

A



AAA Batteries (3) & Remote Control (1)

B



Bed Legs &Bottom Caps (6)

C



Power Cord (1)
& Power Supply (1)

D



Sync Cable (1)

E




Tandem Bracket (1)
For TXL/CKS Only

F



Retainer Bar (1)
Attached To The Bed Frame

Overview & Parts List

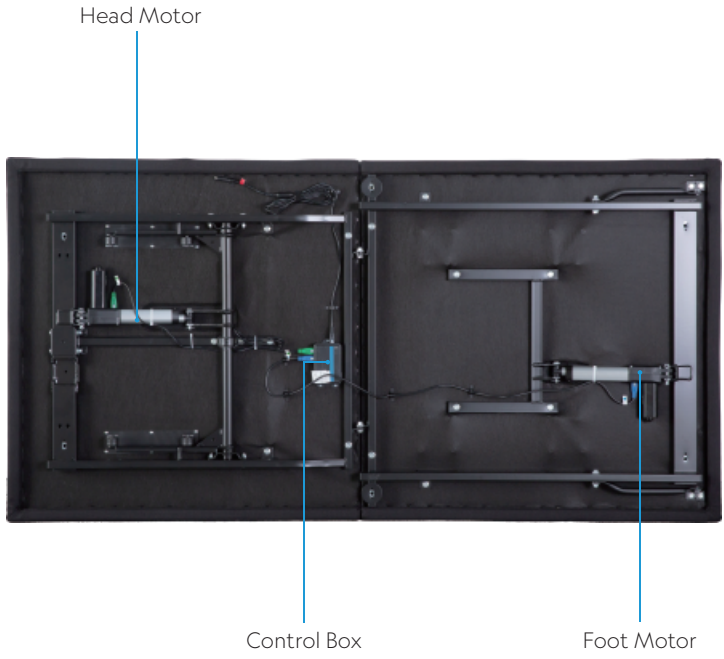

Installation Guide


Notes

1.



Two people are required to assemble this adjustable base.

2.



Open the carton in the flat position with the bottom facing up, to avoid damage.

Step 1

Remove folded bed base from the box and carefully unfold it top-side down on the floor.



Use caution to avoid pinning fingers or any underside wires along the hinge.

Step 2


Open the accessories bag and ensure all accessories are included (see page 4).

Attaching Bed Legs

Step 1

The bed legs come in four segments (3", 3", 3", 3"). These segments can be combined to achieve different heights, allowing you to adjust the base to match your bed frame.

Hand-tighten the legs by threading them clockwise into the pre-threaded holes on the bed frame.

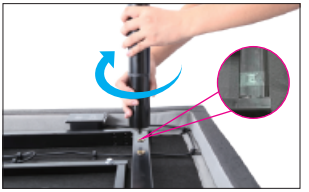

The nut on the frame is removable and replaceable. Please remove the tape on the nut to install legs.

Step 2

Once the legs are attached, pick up the base from the head and foot and flip it over, being careful not to rest it on the legs.

Installation Guide

Installing Retainer Bar

Step 1

With assistance turn the bed frame over, top side up.



Step 2

Insert the ends of the retainer bar into the quick connect brackets located at the foot of the bed.

Setting Up Electronics

Step 1

Take out the power supply and power cord from the accessory box.



Step 2

Connect the power cord and plug the power cord into a working elecrtrical outlet.




Note: Do not overload the power board.

Step 3

Install the three (3) AAA batteries into theremote control. Confirm the remote controlworks by pressing the lift buttons.



Remote Control Instructions

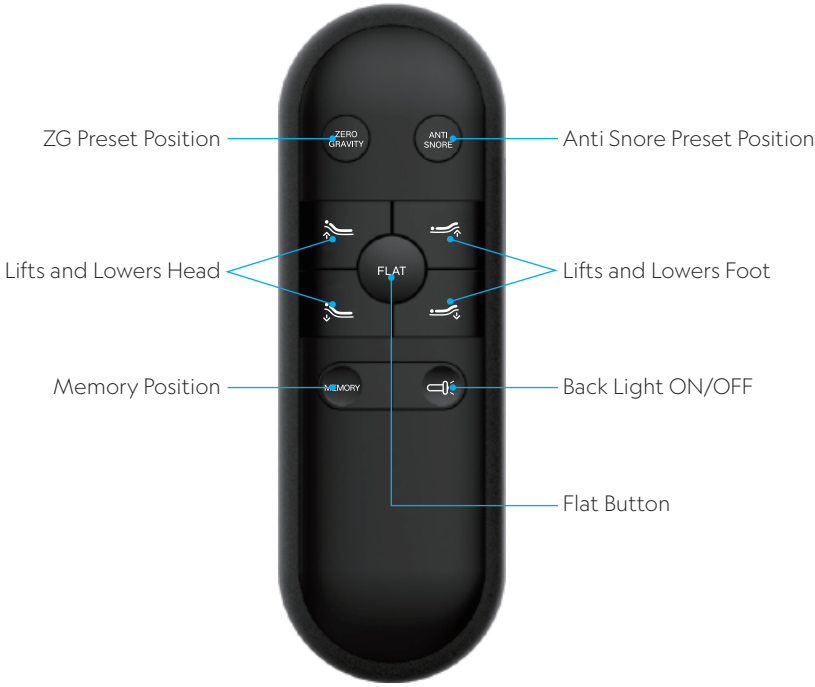

Pairing Remote Control Instructions

The original remote that comes in the box, should already pair with the base.
In the eventthat the remote is not paired with the base, follow these steps.

Remote Is Not Paired With The Base


STEP 1

Make sure the batteries in remote work fine.
Replace them when necessary.



STEP 2

Plug the power cord to the power source.



STEP 3

Press & hold buttons of head up and foot up simultaneously, and then press & hold the blue button on the cord that connected to the power supply.
Once you hear beeps, it is paired.





Synchronizing Two Bases - Unison Movement

Using the Sync Cable

As an alternative to wirelessly synchronizing bases with your remote, you can use the Sync Cable to synchronize two adjustable bed bases.

1. Set two bases next to each other.
2. Locate the Sync Cable Input on the Control Box of each base.
3. Plug the Sync Cable into each bases.
4. Test the connection by moving each base with your remote control.






Tandem Bracket Installation

(King, Cal King only)

A connecting strap is included with TXL & CKS bases. If installing a split setup, optional plastic connecting straps can be used to help secure the bases together.


STEP 1


With the bases in their desired location, slightly loosen both legs to allow the strap to fit on the leg bolt, between the leg and frame.

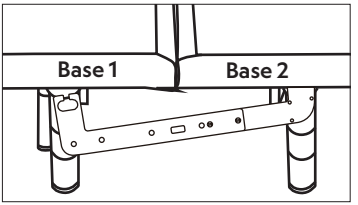

STEP 2

Slide sides (a) of the connecting strap onto leg bolt. Secure the strap by shifting to the left.

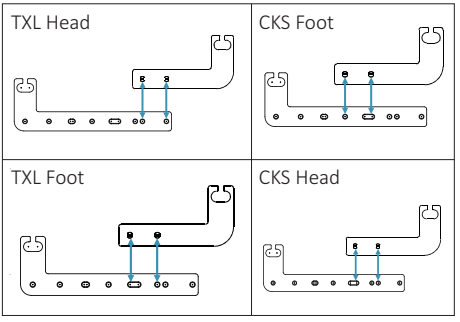

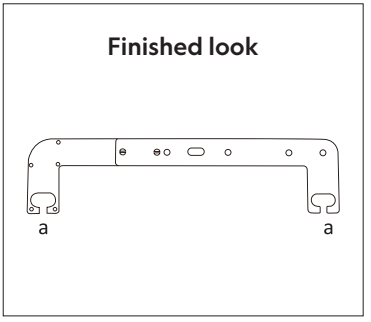

STEP 3

Re-tighten legs. Do not over tighten. Use the remaining strap and repeat on other end of the base.

Troubleshooting

In the event that the power foundation fails to operate, assess the symptoms and possible solutions provided in the chart below.


Remote control illuminates and appears to be operable, but will not activate bed.	Verify that the power cord is plugged into a working, grounded electrical outlet. Test the outlet by plugging in another working appliance.
The base's power features will not activate.	Program the remote control (see the Setting Programmable Positions and Pairing Remote section of this manual for programming procedures). Unplug the power cord, wait 30 seconds, and plug it back in to reset the electronic components. The surge protection device or the electrical outlet may be defective. Test the outlet by plugging in another working appliance.
Wireless remote will not illuminate.	Replace the batteries in the wireless remote.
Head or foot section will elevate, but will not return to the horizontal (flat) position.	Bed mechanism may be obstructed. Elevate the bed and check for an obstruction. Remove the obstruction. The head section may be too close to the wall. The headboard may be too close to the edge of the mattress. Verify that there is enough distance between the headboard brackets and the mattress. Adjust if required.

Troubleshooting

Head and Foot lift function has minor interference during operation.	Check batteries in the wireless remote control, replace with three (3) new AAA batteries if necessary. Make sure that you are following the duty cycle of the motors (do not operate more than two minutes over an 18-minute period, or approximately 10% duty cycle). Press the lift buttons squarely and accurately. The wireless remote control may be experiencing common Radio Frequency Interference from other radio transmitting devices. Wait several seconds, and then try pressing the appropriate button again. See the FCC Compliance Statement on page 5 of this guide.
A clicking noise is heard under the bed when raising or lowering.	This is normal. The lift motor relays “click” when they are engaged. No action is required.

Contact US
We're here to help you.

If you have any issues with this product, please don't hesitate to reach out to us via email .

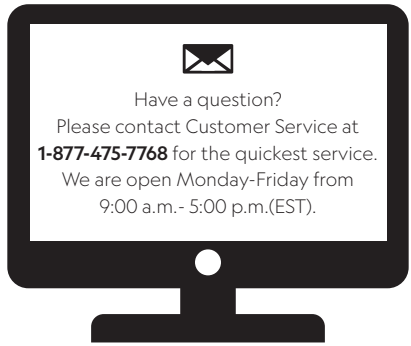

We want you to be completely satisfed with your purchase!
If anvthing is missing, damaged, incrrect, or not what you expected, don't worry.
Please keep the outer packaging and take photos of the packaging and products, then reach out to us at **csr@mlilyusa.com.**
We assure youthat we will address your concerns and provide a solution within 24 hours.

For this product, We offer two years of free local after-sales service (electric motors and electronic control parts) and twenty years of paidafter-sales service.