
尺寸A5 128g铜版纸 3折页风琴折

User Manual

LIFT SLING

Model: JY-BKK-402A

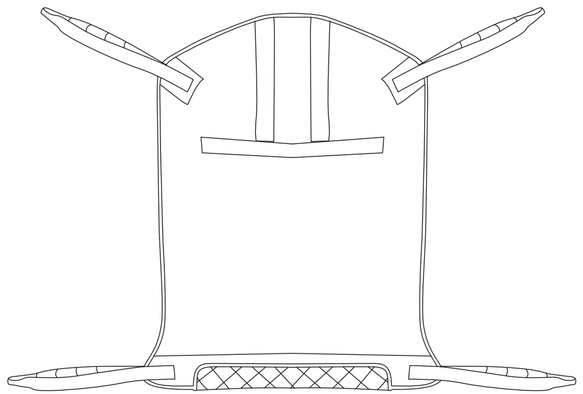

Maximum load: 230kg.

Safety Warning

Please read the instructions carefully before using this product.

Failure to follow the instructions may cause harm to you and others.

Product introduction

This sling is designed with head support and can wrap the body well, greatly improving comfort. It can also help caregivers to carry and transfer patients in different scenarios.

For example, this product can be used when the patient is sitting or lying, when the patient needs to go to the toilet or take a shower, when the patient is in bed or on a chair (wheelchair), etc., which is convenient and safe.

This product is a hanging version and needs to be used with a crane or lift with a hook.


Safety instructions

1. Before use, check whether the sling is damaged or the sewing thread is loose. If so, stop using it.
2. Make sure the patient's weight does not exceed the safe load of this product.（230KG/ 507 IB）
3. Before using this product, you need to understand and be familiar with the operating instructions of the lifting equipment.

Precautions before and after use

1. Before use, make sure the product model is correct and the operator must fully understand the operating procedures of the lifting equipment.
2. Before using the product, you need to read this manual and the manual of the lifting equipment.
3. When the product is dirty, it must be cleaned before use.
4. After use, check whether the appearance of this product is damaged and whether the sewing thread is loose.
5. After use, check whether the appearance is dirty. If so, please clean it immediately.
6. Please keep this product in a dry environment before and after use.

How to use the product

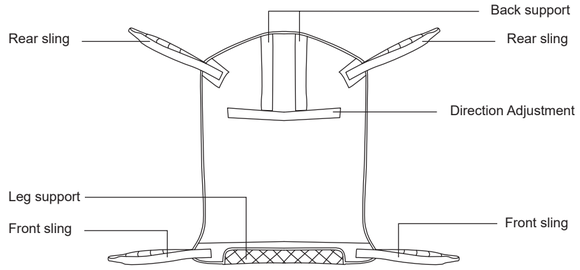

On the bed

1. Place the product on the patient longitudinally.
2. Turn the patient or use a sliding cloth to place the product under the patient. Make sure the center line of the product is flush with the patient's spine, and the arms and legs are inside the product.
3. Hang the crane boom frame directly above the patient.
4. Hang the 4 left and right straps on both ends of the hanger bar and fix them. The two rear straps are hung on the hooks on the left and right sides above the head.The two front slings are hung on the hooks on the left and right sides above the feet.
5. Carefully check and adjust the patient's position to make it the most comfortable position.
6. Slowly raise the hanger bar to straighten the 4 straps and check whether the straps are firm.
7. Operate the crane carefully and always pay attention to the patient's position and status.
8. After transferring the patient to the predetermined position, slowly lower the hanger bar until the 4 straps are in a relaxed state, and then remove the straps.

On the chair

1.Gently tilt the patient's upper body, then place the product behind the patient (if necessary, you can also use a sliding cloth to assist), making sure the center line of the product is flush with the patient's spine, and the arms and legs are inside the product.
2. Hang the crane boom frame directly above the patient.
3. Hang the 4 left and right straps on both ends of the hanger bar and fix them.
4. Carefully check and adjust the patient's position to make it the most comfortable position.
5. Slowly raise the hanger bar to straighten the 4 straps and check whether the straps are firm.
6. Operate the crane carefully and always pay attention to the patient's position and status.
7 After transferring the patient to the predetermined position, slowly lower the hanger bar until the 4 straps are in a loose state, and then remove the straps.

Product life

The life of this product depends on the number of uses and the number of washing cycles. When washed once a week, the life of this product is 2 years. 2. Unopened products can be stored in a dry and clean environment for 3 years.

Washing method

Do not bleach.	Do not iron.	Please read the precautions carefully.
Tumble drying can be used. Lower temperature, maximum exhaust temperature 60˚C (140˚F).	80˚C	Maximum washing temperature 80˚C (176˚F).

Baoding junyao medical treatment manufacturing co.,ltd
Da Zhuang Zhen Xie Zhuang Cun,
Qingyuan District, Baoding City. Hebei Province

Made in China